


Tue Sep 26 12:14:17 2006


TIDE Mass_1

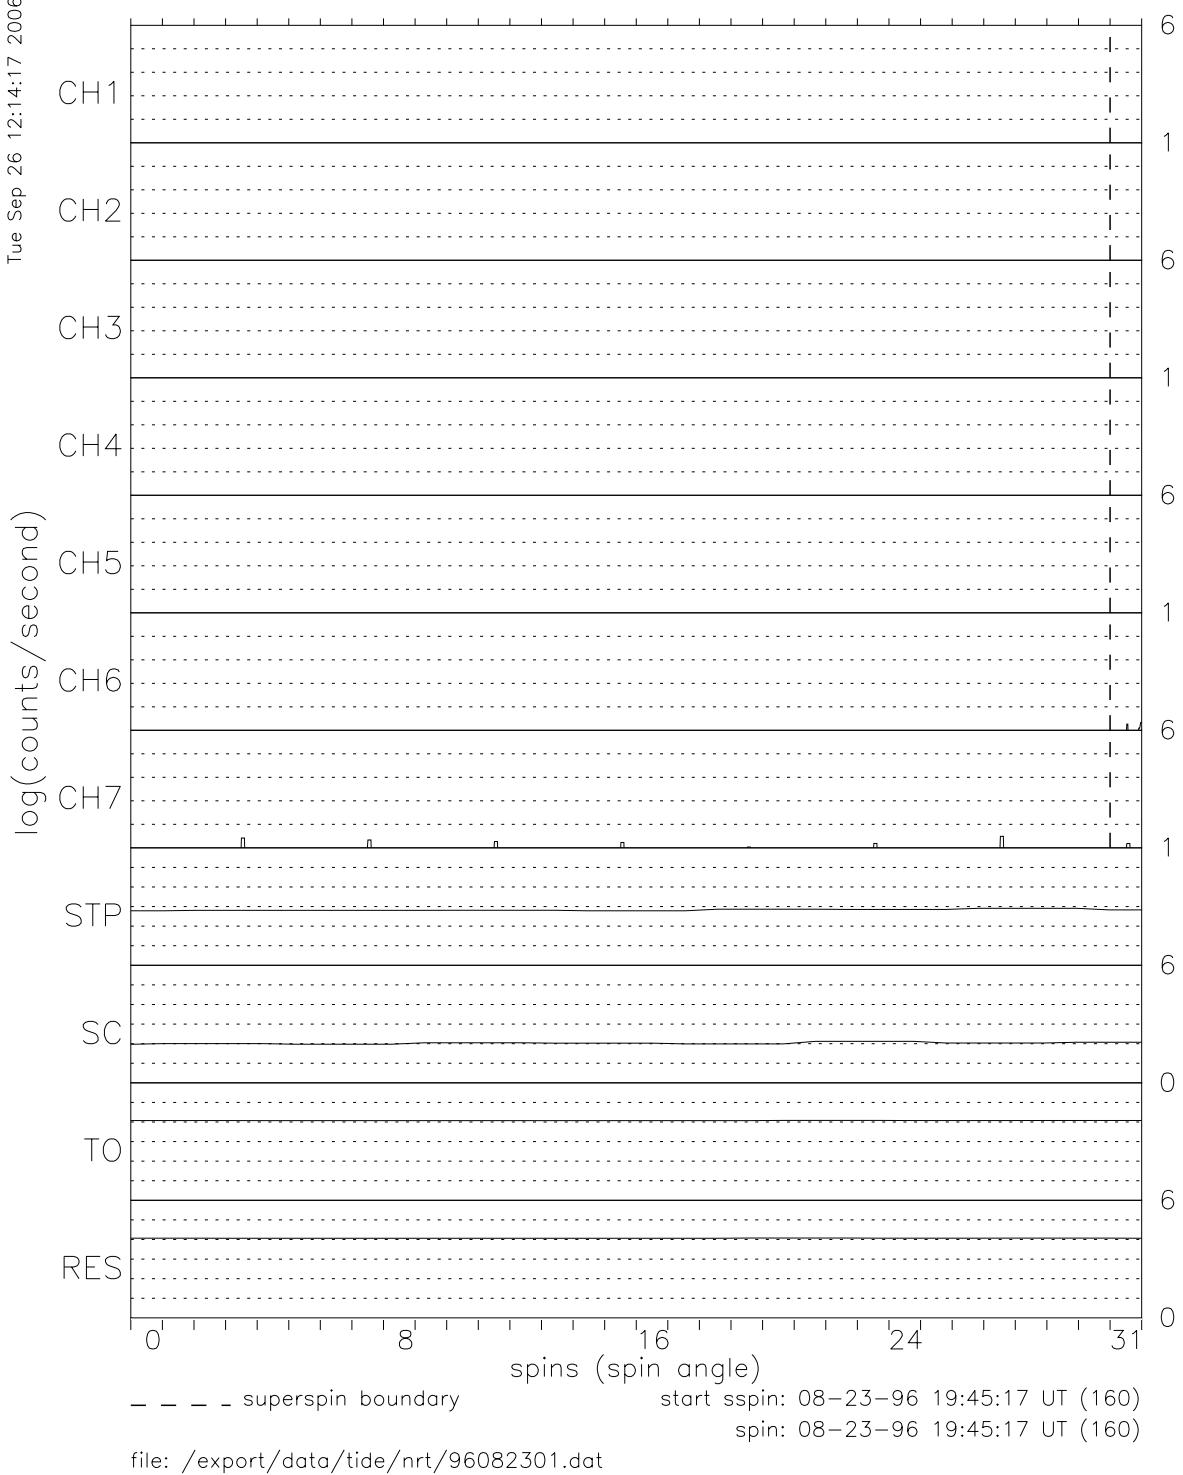

-15kV TOF: -9051 v
-3.6kV MCP: -2672 v
-2.4kV MCP: -1610 v
Input Cur: 306 ma
RPA max: 236 v
Mirror max: 238 v

Tue Sep 26 12:14:17 2006

TIDE Direct Events

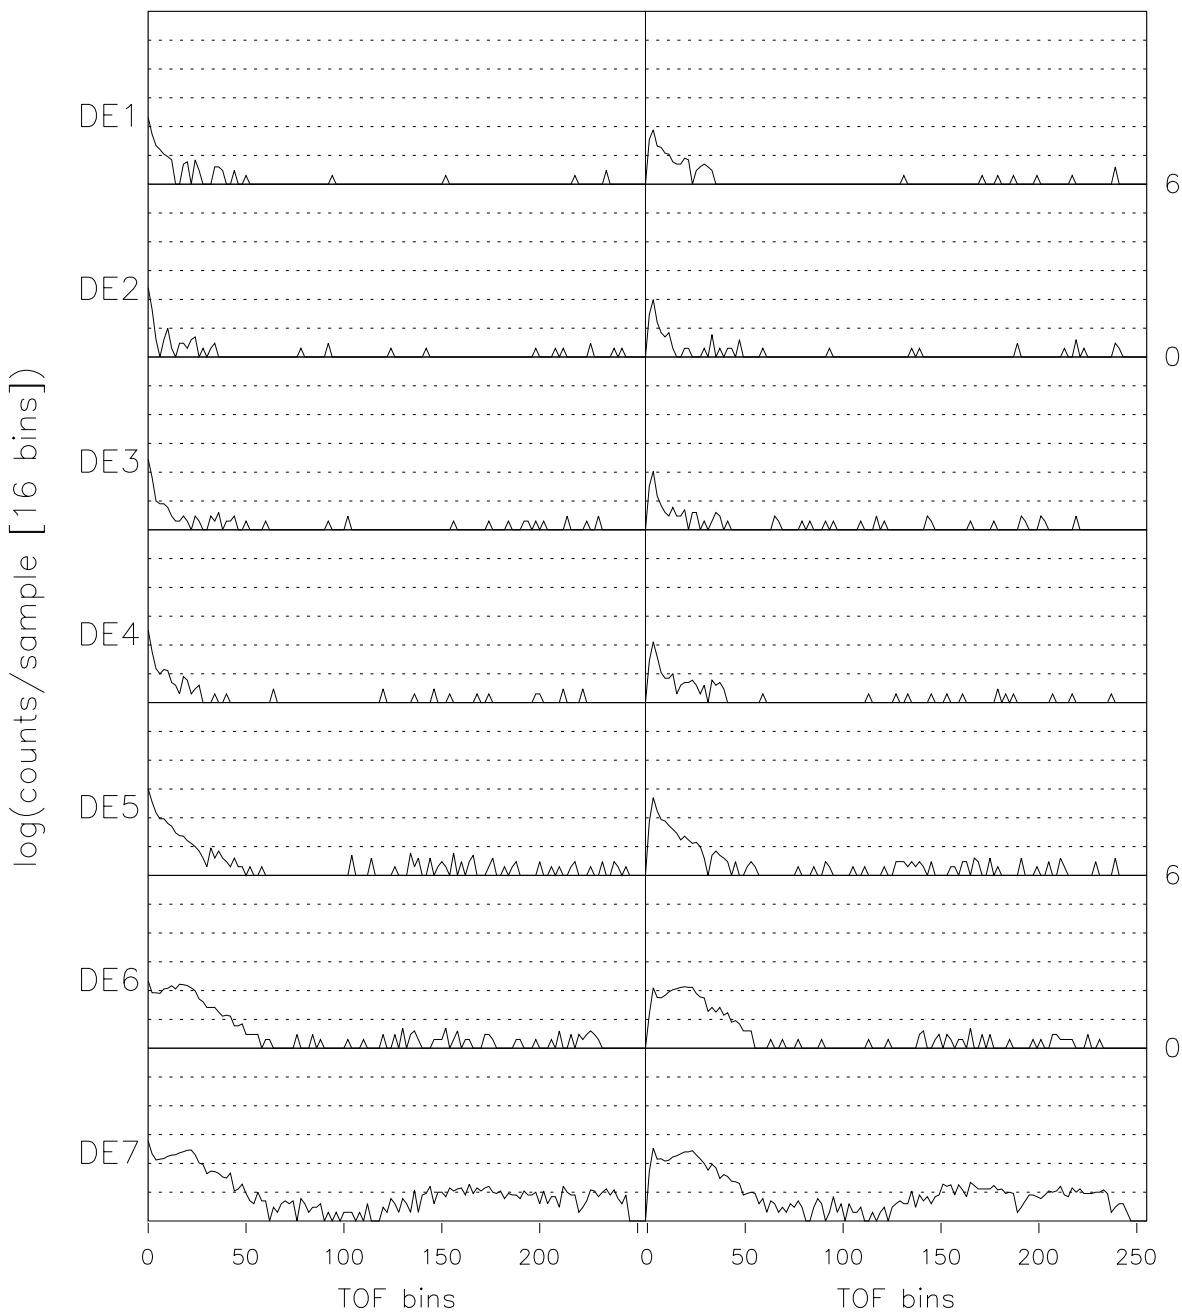

reported: 08-23-96 19:38:49 UT

reported: 08-23-96 19:42:00 UT

file: /export/data/tide/nrt/96082301.dat

-15kV TOF: -9181 v
-3.6kV MCP: -2672 v
-2.4kV MCP: -1620 v
Input Cur: 304 ma
RPA max: 236 v
Mirror max: 238 v